

CLV61x

Bar Code Scanner

CLV610-C0000 CAN Mid Range
CLV615-F2000 FIELDBUS Long Range

SICK
Sensor Intelligence.



Intended Use

The CLV61x bar code scanner is an intelligent SICK IDpro sensor and is used exclusively for automatic, stationary identification and decoding of bar codes on moving or stationary objects. The data content of the decoded bar codes is sent by the CLV61x to a superordinate computer for further processing. Depending on the model, this is either done directly via a serial data interface (RS-232) or indirectly via the SICK CAN scanner network on a coordinating device (e.g., master).

Correct use also includes compliance with all information in these operating instructions as well as in the supplementary [“CLV61x Bar Code Scanner” Technical Information](#) (no. 8015592).

The product family CLV61x consists of the three series ECO, CAN, and FIELDBUS (FIELDBUS in combination with the optional CDF600-21xx fieldbus module). Depending on the model, the series offer the following options:

- Reading range variants (e.g., Short Range, Long Range)
- Line scanner or raster scanner
- Reading window on front or side
- Different connecting cable lengths

All devices have two serial data interfaces (HOST/AUX). The CAN and FIELDBUS series also offer the SMART decoder for

identifying partly damaged or low-quality bar codes as well as an additional CAN interface.

About This Document

The purpose of these operating instructions is to allow you to put the CLV61x into operation quickly and easily and to achieve initial read results as a stand-alone device.

The operating instructions describe the commissioning process for an application with a **single** CLV61x. This is done, for example, using the device version CLV610-C0000 from the CAN series and its default setting. The CDB620 connection module, for example, is used for the industrial-standard signal distribution of the CLV61x.

The operating instructions are valid for the following variants:

- CLV610-C0000 (CAN, Mid Range, line scanner, reading window on front, SMART decoder)
- CLV615-F2000 (FIELDBUS, Long Range, line scanner, reading window on side, CAN, SMART decoder)

In the following, the bar code scanner CLV61x is referred to in simplified form as “CLV61x.”

Supplementary Documents

More detailed information about mounting and electrical installation as a stand-alone device is available in [“CLV61x Bar Code Scanner” Technical Information](#) (no. 8015592). This document describes:

- Optional mounting accessories (brackets)
- The prevention of ground potential equalization currents in applications with widely distributed systems
- Pin/lead color assignments of cables
- Electrical wiring plans for the CDB620 connection module relating to the CLV61x

Operation of the CLV61x CAN in the SICK CAN Sensor Network

The setup and wiring of the SICK-specific CAN network as well as the integration of the CLV61x CAN and FIELDBUS series in the network is described in the [SICK CAN Sensor Network for IDpro Sensors Operating Instructions](#).

Operation of the CLV61x FIELDBUS in PROFIBUS

The integration of the CLV61x FIELDBUS series in PROFIBUS via the CDF600-21xx fieldbus module is described in the [“CDF600-21xx Fieldbus Module PROFIBUS” Operating Instructions](#) (no. 8015335) and the supplementary [“CDF600-21xx Fieldbus Module PROFIBUS” Technical Information](#) (no. 8015337).

Information about configuration can be found in the online help function of the configuration software SOPAS ET.

The information can be accessed as a PDF on the enclosed data carrier (“Identification & Measuring Manuals & Software” DVD) or on the CLV61x product site on the web (www.mysick.com/en/CLV61x).

For viewing on a PC, PDF visualizing software such as Acrobat® Reader® (<http://get.adobe.com/reader>) is required.

Safety Information

- This chapter is about the safety of commissioning personnel, as well as operators of the system in which the CLV61x is integrated.
- Read these operating instructions before starting any work on the CLV61x in order to familiarize yourself with the device and its functions. The operating instructions are considered a part of the device and must be kept in an accessible location in the immediate vicinity of the CLV61x at all times!
- The CLV61x corresponds to laser class 2. Laser warning notice → see *“Risk of Injury from Laser Radiation! Page 6”*.
- Opening the screws of the CLV61x housing will invalidate any warranty claims against SICK AG. For further warranty provisions, see the General Terms and Conditions of SICK AG, e.g., on the delivery note of the CLV61x.

Commissioning and Configuration

Scope of Delivery

Per CLV61x

- CLV61x in the ordered version (series, reading range, scanning method, reading window orientation)
- 1 set laser warning label in German/US English and French/US English to cover the US English laser warning label on the type label as required
- “Identification & Measuring Software & Manuals” DVD (no. 2039442)
- Printed operating instructions in German (no. 8015588) and English (no. 8015589), in other languages as a PDF on the DVD if applicable
- Technical information in German (no. 8015591) and English (no. 8015592) as a PDF on the DVD

Accessories

- Accessories that can be optionally ordered such as brackets/cables

Step 1: Mounting

NOTE

Radio interference may occur when the CLV61x is used in residential areas!

- The CLV61x must be used exclusively in industrial environments.

Equipment Required

- 2 x M5 screws for mounting the CLV61x on a mounting device (bracket). Screw length is dependent on the mounting base (wall thickness of bracket). When using optional SICK brackets, screws for the CLV61x are included.

Mounting Requirements


- The permitted ambient conditions for the operation of the CLV61x must be complied with (e.g., temperature, radi-

ated emission, ground potential → see section *“Technical Specifications (Excerpt) Page 5”* and section *“Risk of injury/risk of damage via electrical current! Page 2”*).

- The device must only be mounted using the pairs of threaded mounting holes provided for this purpose.
- Stable mounting device with sufficient load-bearing capacity and suitable dimensions for the CLV61x. Weight depends on model, max. 206 g/7.27 oz. (not including cables). For dimension drawing, → see section *“Device overview CLV61x”* on page 3.
- Shock and vibration-free mounting.
- Clear view of the bar codes to be measured on the objects.


Mounting CLV61x

1. Depending on the country of use, cover the English laser warning label with one of the provided language versions (German or French) if required.
2. Select a suitable mounting location for the CLV61x with a clear view of the object to be scanned. The mounting location and position depend on the respective reading range of the CLV61x version. The available reading range is dependent on the distance from the code and the required resolution. The mounting location must therefore be chosen whilst taking into account the respective reading field length and height, as well as resolution and depth of focus (→ see section *“Reading fields Page 5”*).
3. Mount the CLV61x on a bracket using both screws.

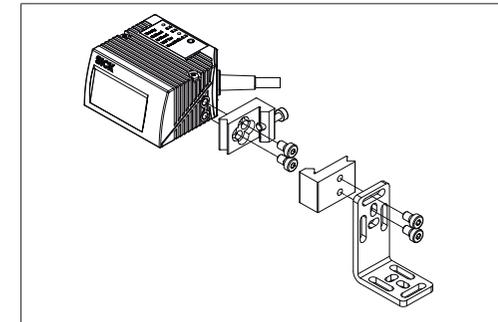


Mounting example: use of quick-clamping device (clamp bracket) no. 2025526 in combination with the mounting bracket no. 2020410

4. Depending on the scanning method, roughly align the CLV61x on the object with the bar code to be measured.

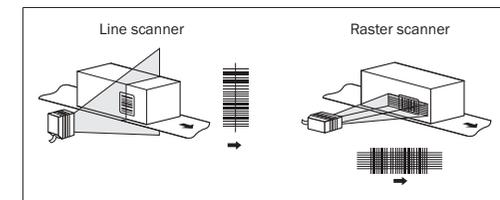

Allocation of scanning method to bar code and conveyor direction

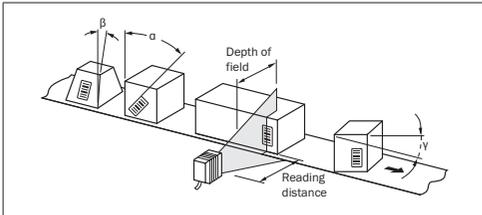


Possible read angle that could occur between scanning line and bar code

Angle	Limit Value
Tilt α	max. 30° *)
Pitch β	max. 45°
Skew γ	max. 45°

*) depending on the module width

- In order to avoid a total reflection of the scanning line, tip the CLV61x with the following skew angle from the perpendicular to the bar code surface.

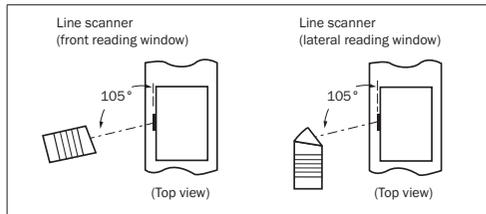

Avoid surface reflection through correct arrangement

Connection Module CDB620

- Mount the CDB620 connection module in the vicinity of the CLV61x. Through the serial data interfaces (RS-232) recommended max. distance 5 m/16.4 ft. Mount the CDB620 in such a way that the device can be accessed at all times. In relation to this, see "CDB620 Connection Module" Operating Instructions (no. 8012119), which are enclosed in printed form with the device.

Step 2: Electrical Connection

- The electrical installation must only be performed by qualified electricians.
- The currently applicable safety regulations must be observed when working in electrical systems!
- Electrical connections between the CLV61x and other devices may only be created or fixed when there is no power to the system. Otherwise, the devices may be damaged.
- When using extension cables with open ends, ensure that bare wire ends do not come into contact with each other (risk of short-circuit when supply voltage is switched on!). Wires must be appropriately insulated from each other.
- Wire cross sections of the supply cable from the customer's power system should be designed in accordance with the applicable standards.
- If the supply voltage for the CLV61x is not supplied via the optional CDB620 connection module, the CLV61x must

- be protected by a separate max. 2 A slow-blow fuse at the beginning of the supply circuit.
- In order to retain the IP 65 enclosure rating for the CLV61x connecting cable even when using an extension cable (e.g., no. 6034417, 2 m/6.56 ft), insert rubber seal no. 4038847 between the plug and socket of the D-Sub plug connection of the cables and screw in the plug connection.
- Circuits connected to the CLV61x must be designed as SELV circuits (SELV = Safety Extra Low Voltage).


⚠ DANGER

Risk of injury/risk of damage via electrical current!

The CLV61x is designed to be operated in a system with professional grounding of all connected devices and mounting surfaces to the same ground potential. Incorrect grounding of the CLV61x can, due to equipotential bonding currents between the CLV61x and other grounded devices in the system, place the metal housing under a dangerous voltage, cause malfunction and destruction of devices as well as damage to the cable shielding through heating, and thus cause cable fires.

- Work on the electrical system must only be performed by qualified electricians.
 - Ensure ground potential at all grounding points.
 - In the event of damage to the cable insulation, immediately switch off the power supply and have the damage repaired.
- See the "Electrical Installation" chapter in the "CLV61x Bar Code Scanner" Technical Information (no. 8015592) on the DVD or on the product site on the web (www.mysick.com/en/clv61x) for measures to eliminate hazards.

- Connect the 15-pin D-Sub-HD plug of the CLV61x cable to the CDB620 connection module.
- Connect a read pulse sensor, such as a photoelectric sensor at the "Sens 1" switching input of the CDB620. See the "Electrical Installation" chapter in the "CLV61x Bar Code Scanner" Technical Information (no. 8015592).
- Connect the serial AUX interface (RS-232) of the CLV61x to the PC (9-pin D-Sub plug) with a suitable data cable (e.g., no. 2014054, 2 m/6.56 ft) using the internal plug "AUX" (9-pin D-Sub) of the CDB620. If the PC does not have an RS-232 interface, use a suitable adapter cable with RS-232 <-> USB converter (e.g., no. 6042499, 1.5 m/4.92 ft).

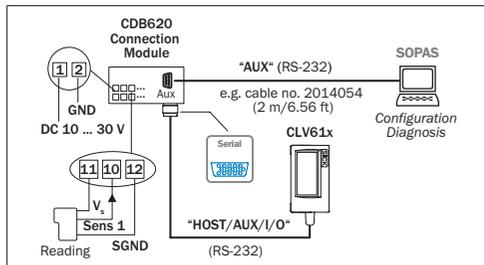

Electr. connection of the CLV61x for commissioning as a stand-alone device

Switch on the supply voltage for the CDB620 and the PC.

All LEDs on the CDB620 will light up briefly. The CLV61x starts with a delay and uses the default parameters set in the factory for the initialization. After a successful self-test, the LED on the CLV61x lights up blue to indicate the "Device Ready" status.

Step 3: Configuration with PC

User Modes/Statures of the CLV61x:

- Quick Start (initial commissioning for read operation)
- Read operation
- Percentage evaluation (for diagnostic purposes)
- Configuration via SOPAS ET configuration software
- Firmware download


Configuration

In case of error, the SOPAS ET configuration software is used by default to adjust the CLV61x parameters to the application and to the diagnostics.

Installing and Starting the Configuration Software

- Install the SOPAS ET software on the PC from the enclosed "Identification & Measuring Software & Manuals" DVD (alternatively, download and install it from the website "www.sick.com/software" Softwaretyp SOPAS ET). In this case, select the "Complete" option as suggested by the install wizard.
- Start program option "SOPAS Single Device". Path: Start > Program Files > SICK > SOPAS Engineering Tool > SOPAS (Single Device)
- Establish a connection between software and CLV61x e.g., via the serial AUX interface (57.6 kBd). The connection wizard starts automatically. Under interface selection, select the standard protocol.
- Select the CLV61x from the devices that are now available and displayed. The QUICK START device page appears.

SOPAS ET Program Window

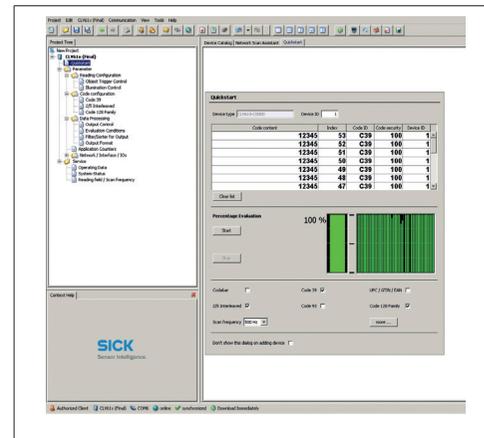

Device tree (left), device page QUICK START (right)

User Level, Parameter Download

The user is automatically logged onto the CLV61x at user level "Authorized Client" (password: client). The user can change parameters, which will be immediately transferred to the CLV61x (default). Initially they will have only temporary effect there, without being saved, until the supply voltage is switched off. If the parameters are to be retained, they must be permanently saved (➔ see section "c. Completing the Configuration Page 2").

a. Configuration via the "Quickstart" Device Page

The "Quickstart" device page offers an overview of the most important parameters and enables quick evaluation of code content. Functions such as "Evaluation Window," "Percentage Evaluation," "Code Configuration," and "Scanning Frequency" are available via the Quickstart.

Evaluation Window

The evaluation window shows the code content, the code type, the increment index, the code security, and the device number of the reading CLV61x.

Percentage Evaluation

The percentage evaluation permanently assesses the quality of the reading. Bar codes are not assessed. Here, the bar codes must not be subjected to any conveying movement.

The CLV61x performs 100 scans in each case and evaluates the reading quality. The CLV61x continuously emits read results every 2 s via the AUX interface, together with the read diagnostic data.

Code Configuration

In the factory default setting, the CLV61x decodes the following code types:

- Code 39
- Interleaved 2 of 5
- Code 128 family

To activate or deactivate further code types: Device tree > Parameters > Code configuration.

b. Summary of Further Useful Adaptation Options

Object Trigger Control

The CLV61x can, as described in the standard application, be operated with a connected read pulse sensor, such as a photoelectric sensor on the "Sensor 1" switching input. To select a different pulse type or switching input: Device tree > Parameters > Object trigger control.

c. Completing the Configuration

- Permanently save the entire configuration: Parameter set in CLV61x: click the button Configuration file on the PC: click the button.

Important!

In order to commission the CLV61x CAN or FIELDBUS series in the SICK CAN scanner network together with further SICK products, select the option SOPAS ET when starting the configuration software program. Path: Start > Programs > SICK > SOPAS ET Engineering Tool > SOPAS.
The SOPAS Single Device option is not suitable for this.

Default Setting CLV61x (Summary)

Parameter	Value
Scanning frequency	500 Hz
Laser timeout	No
Code length	Free (max. 1,500 characters in reading interval across all measured codes)
Reading trigger	Read operation: Start: Sensor 1 switching input Stop: Sensor 1 switching input Quick Start: START and STOP buttons for percentage evaluation
Host interface	57.6 kBd, 8, n, 1, Output format: 1
AUX interface	Output format: read diagnosis
Switching outputs	Result 1: Device Ready Result 2: Good Read
Password protection for parameters	No


Step 4: Fine Adjustment

- Align the CLV61x so that the angle between the scanning line and the bar code stripes is almost 90°.
- Manually guide objects with bar codes successively into the reading field of the CLV61x in a realistic manner and check the reading result. If objects are only guided in an unstructured manner, it may be necessary to check several different positions of the bar codes. Here, it must be ensured that the limit values of the permitted read angles are not exceeded.
- Adjust the CLV61x so that the good read rate is 100%.


Description of the Device

Device overview CLV61x

Reading window on front

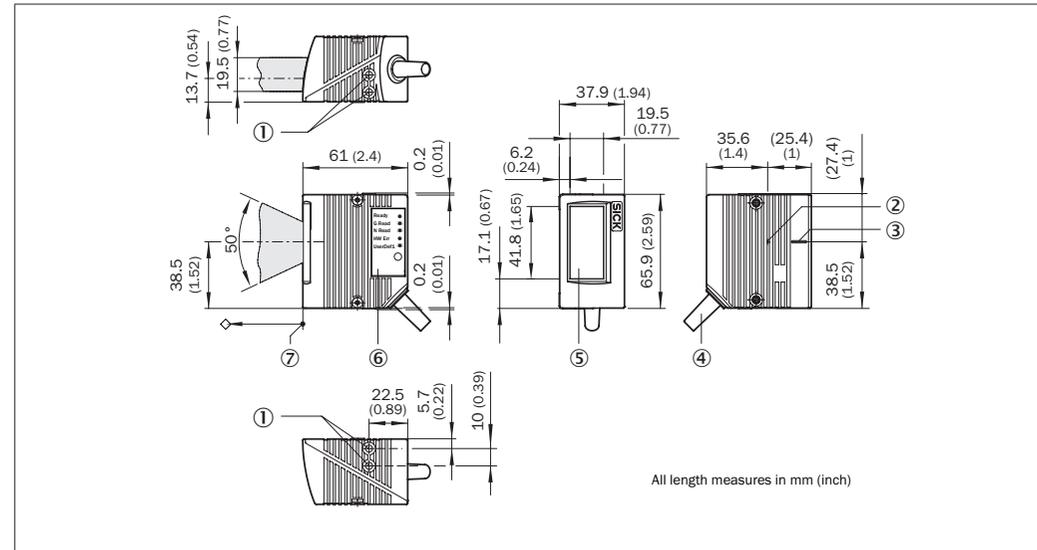


Reading window on side

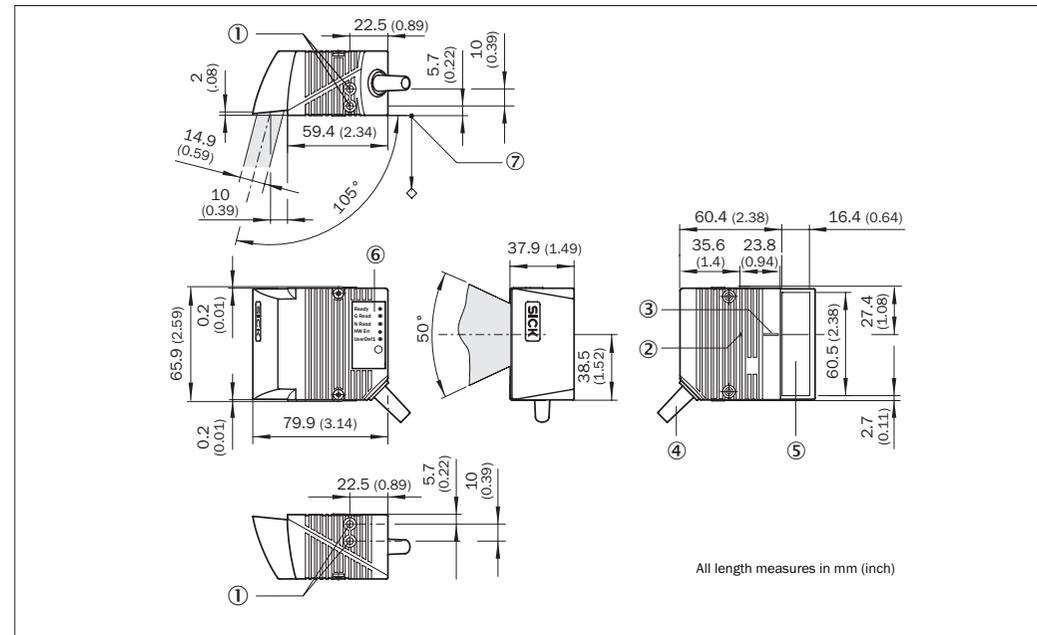

Legend:

- 2 x threaded mounting hole M5, 5 mm deep for mounting the CLV61x
- Internal impact point: rotation point of the variable direction laser beam
- Central position of the deflected laser beam in the V-shaped aperture angle
- Cable outlet, standard cable 0.9 m/2.95 ft (+10%) with 15-pin D-Sub-HD plug
- Reading window
- Status display (1 x RGB-LED) with signal color allocation
- Reference point for reading distance (housing edge) from CLV61x to object

Optical Status Indicators

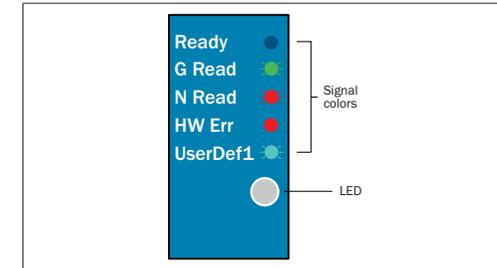


Indicator colors and behavior of LED status display


Indicator	Color of LED	Status
Ready	Blue	Lights up constantly after switching on and completion of successful self-test.
	-	Goes out when downloading configuration data from the CLV61x
G Read	Green	Lights up briefly after Good Read
N Read	Red	Lights up briefly after No Read
HW Err	Red	Lights up constantly in case of hardware error
Further indicators	Red Blue	Firmware download: Indicator flashes alternately
	Red	Firmware download: Lights up constantly in case of error

● = lights up constantly or once briefly
●● = flashes, ●●● = flashes alternately


Overview of all interfaces and connection options for CLV61x ECO/CAN

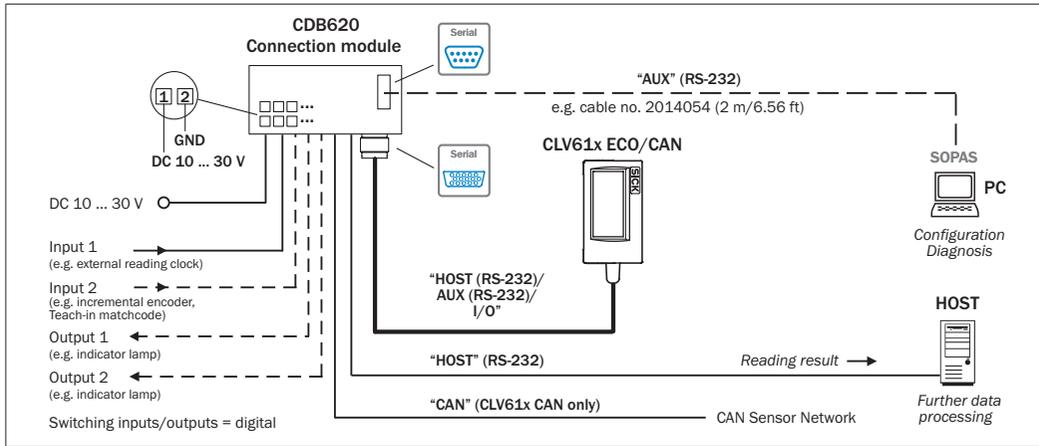

Overview of all interfaces and connection options for CLV61x FIELDBUS

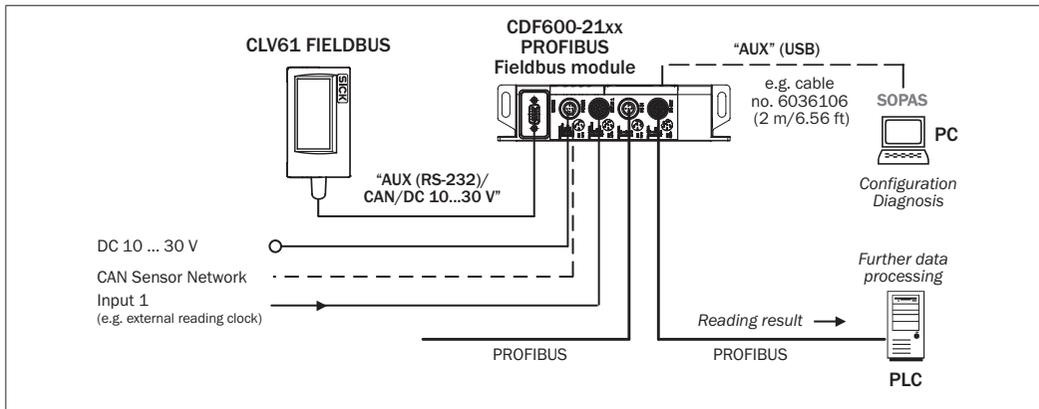


Overview of pin assignment

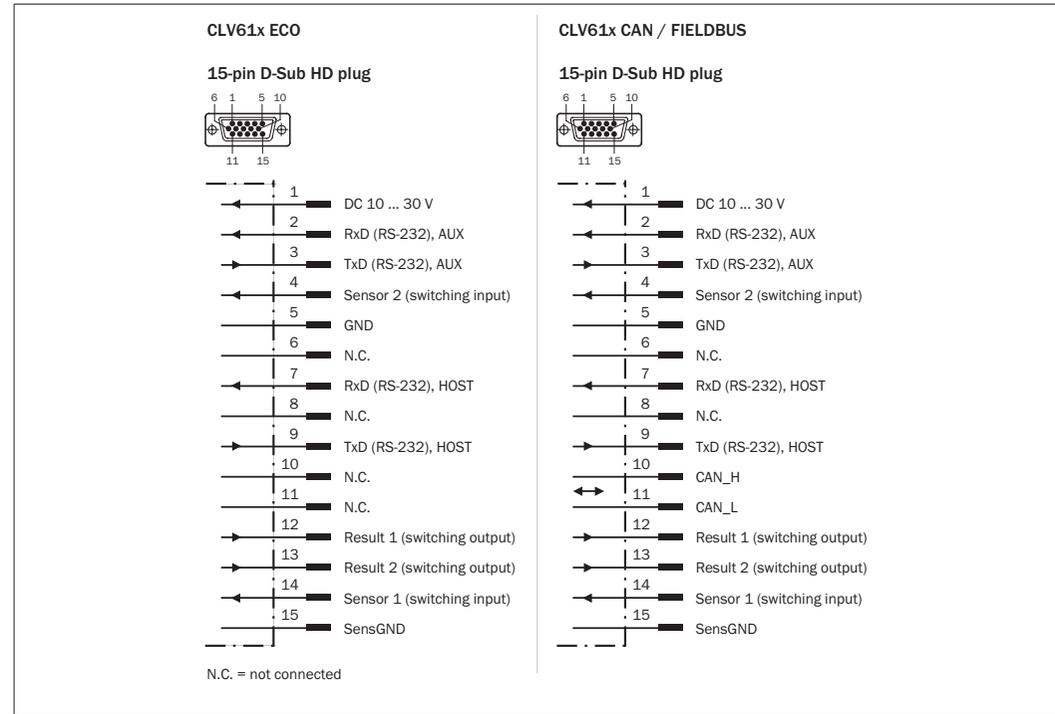


Reading fields

CLV610: Mid Range, reading window on front

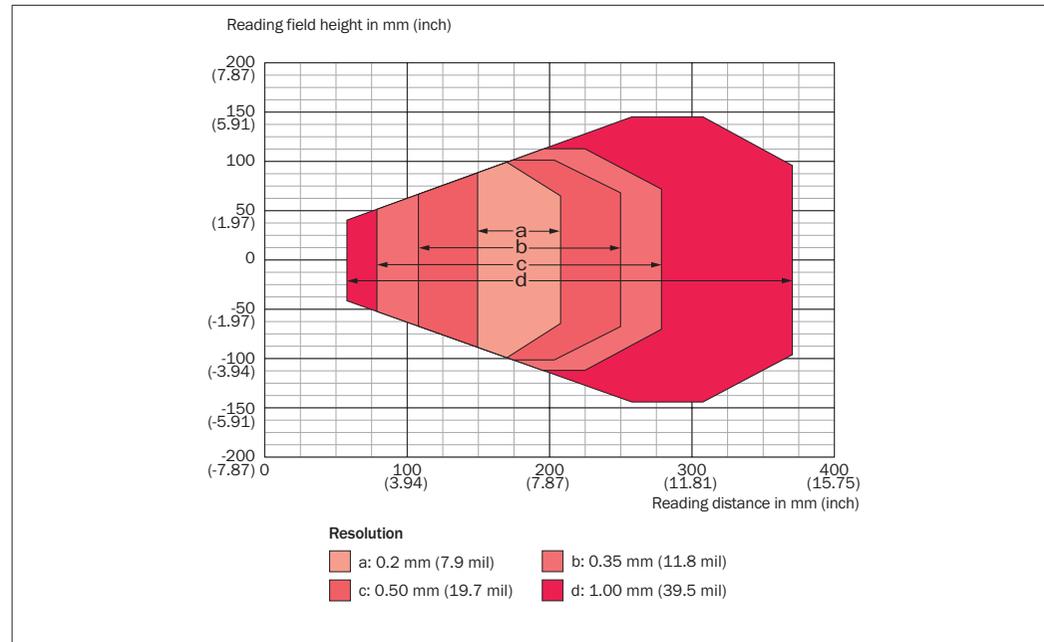

CLV615: Long Range, reading window on side

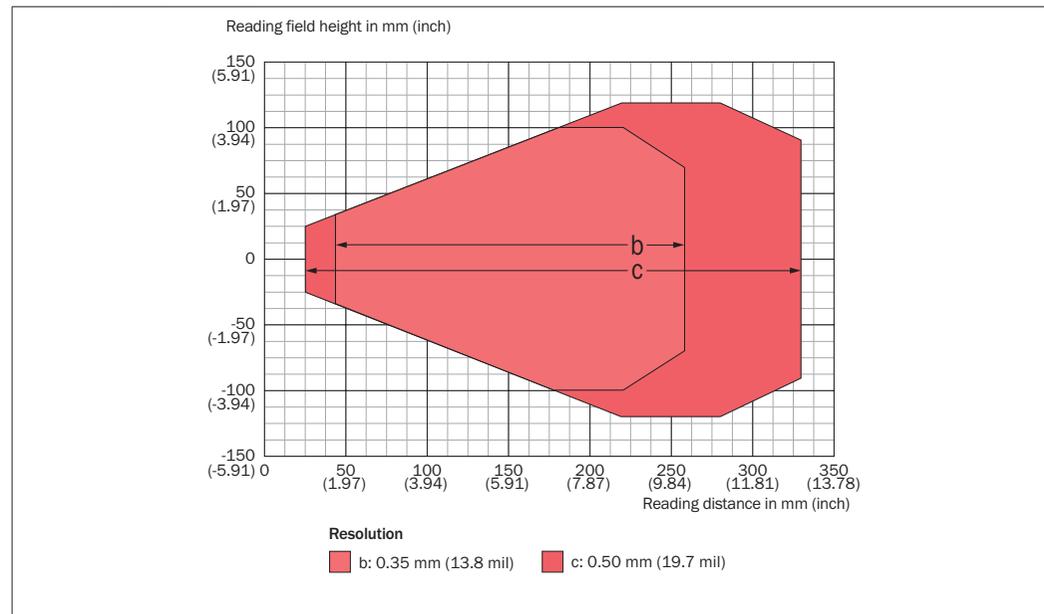

Acoustic Status Indicator (Beeper)

Depending on the user mode of the CLV61x, the beeper uses different melodies or single tones to indicate the following results:

- Fulfillment/non-fulfillment of a configured condition in read operation (e.g., Good Read)
- The completion of device functions triggered by the user or ended by quitting (confirmation of operation steps)
- Completion of functions (positive/negative confirmation)

User Mode	Function/Sound
Switching on	Successful self-test and start of read operation: melody
Read operation	Confirmation of Good Read in default setting: a tone. Adjustable event condition ^{*)}
Percentage Evaluation	Start: melody 100 scans per read: a tone End: melody
Configuration	Parameter download to CLV61x: Start: melody, successful completion: melody Parameter upload from CLV61x: no sound
Firmware download	Firmware: Start: a tone, successful completion: a tone Reboot CLV61x: Successful completion: melody Loading the sdd file to the CLV61x: Successful completion: melody

*) Allocation, e.g., via configuration software SOPAS ET

Beeper Default Setting:

Switched on, volume: quiet, read operation: output condition "Good Read".

Technical Specifications (Excerpt)

Models	CLV610-C0000 (no. 1057125) CLV615-F2000 (no. 1058334)
Series	CLV610-C0000: CAN CLV615-F2000: FIELDBUS
Scanning method	Line scanner
Reading window	CLV610-C0000: on front CLV615-F2000: on side
Reading range/ Code resolution	CLV610: Mid range/ 0.2 ... 1.0 mm CLV615: Long range/ 0.35 ... 1.0 mm
Code types	All current 1D code types
Focus	Fixed focus
Scanning frequency	400 ... 1,000 Hz
Light source	Visible red light (655 nm)
Laser class	Class 2 in accordance with IEC 60825-1 Ed.: 2007-03/EN 60825-1 Ed. 2: 2008-05. Complies with 21 CFR 1040.10 except for the tolerance according to Laser Notice No. 50 from June 24, 2007.
Ambient light compatibility	2,000 lx (on bar code)
Optical indicators	1 RGB-LED, multi-colored
Acoustic indicators	Beeper, can be deactivated, can be allocated function for event signaling
Host interface	Serial (RS-232), 2.4 ... 115.2 kBd
AUX interface	Serial (RS-232), 57.6 kBd (fixed)
CAN interface	CAN sensor network 20 kBit/s ... 1 MBit/s
Fieldbus connection	CLV615-F2000 only: Via serial interface to external CDF600-21xx fieldbus module (PROFIBUS)
Switching inputs	2 x physical, 2 x additional external via optional CMC600 module $V_{out} = \max. 30 V$, $I_{out} \leq 100 mA$ Opto-decoupled, reverse polarity protected
Switching outputs	2 x physical, 2 x additional external via optional CMC600 module $V_{out} = V_{+} - 1.5 V$, $I_{out} \leq 100 mA$. Short-circuit protected, temperature protected
Electrical connection	Standard cable 0.9 m/2.95 ft (+10%) with 15-pin D-Sub-HD plug
Supply voltage	DC 10 ... 30 V, SELV in accordance with IEC 6034-4-41: 2005. Reverse polarity protected
Power consumption	Typically 2.8 W ¹⁾
Housing (color)/ reading window	Aluminum die casting (RAL 5012)/ Glass (optionally plastic)
Weight²⁾	181 g/6.38 oz. (with reading window on front) 206 g/7.26 oz. (with reading window on side)
Electrical safety	EN 60950-1: 2011-01
Protection class	III (VDE 016 / IEC 10110-1)
Enclosure rating	IP 65 (DIN 40 050)
EMC	Radiated emission: EN 61000-6-4: 2007-01 + A1: 2011 Electromagnetic immunity: EN 61000-6-2: 2005-08
Vibration resistance Shock resistance	EN 60068-2-6: 2008-02 EN 60068-2-27: 2009-05
Ambient temperature	Operation: 0 ... +40 °C/ +32 ... +104 °F Storage: -20 ... +70 °C/ -4 ... +158 °F
Permissible relative air humidity	90%, non-condensing

1) With switching outputs without load
2) Without connecting cable and plug

For detailed technical specifications, see the [Online Data Sheet](#) on the product site on the web (www.mysick.com/en/clv61x).


Warnings

CAUTION

Risk of Injury from Laser Radiation!

The CLV61x uses a red laser diode and corresponds to laser class 2.

The entire reading window is a laser output aperture.

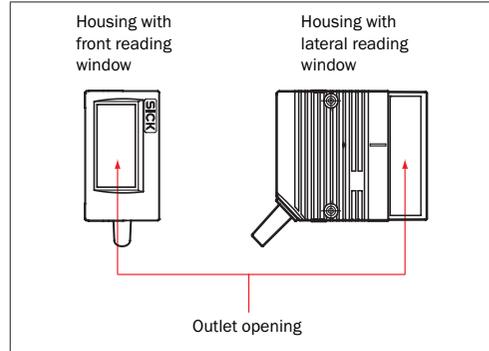

Outlet opening for the laser radiation on the reading window of the CLV61x

The human eye is not at risk when accidentally exposed to the laser radiation for short periods of time (up to 0.25 s). When intentionally exposed to the laser beam for longer periods of time, the retina of the eye may be damaged. The emitted radiation is harmless to human skin.

Caution – incorrect use can lead to the user being exposed to dangerous radiation.

- Never look directly into the beam path (similar to sunlight).
- Never point the laser beam at people's eyes.
- When mounting and aligning the CLV61x, avoid reflections of the laser beam off reflective surfaces.
- Do not open the closed CLV61x housing as this operation will not interrupt possible switching on of the laser diode.
- Comply with the latest version of the applicable provisions on laser protection.

The CLV61x includes two self-adhesive laser warning labels in German or French. These can be stuck over the English text if required.

Important!

Maintenance is not necessary to ensure compliance with laser class 2.



Installation site and design of the combination of black and yellow laser warning label (condition as delivered: English text) and type label with laser performance data.

Controlling the Laser Diode

In real operation (triggered read mode), the CLV61x switches the laser diode on and off again with the trigger signals of the conveyor system (object in reading range). Triggering occurs here via the switching inputs of the CLV61x or by a command via one of the data interfaces.

A laser timeout configured with SOPAS ET (device page ILLUMINATION CONTROL) can be used to automatically switch off the laser diode for this type of object trigger control if the pulse has stopped for too long (e.g., conveyor system has stopped). If the function is activated, the laser timeout is 10 min (default). The current internal reading interval of the CLV61x remains open.

The laser diode is permanently or repeatedly switched on in the following device statuses:

- In the “Percentage Evaluation” and “Auto Setup” user modes (only used temporarily for configuration/diagnosis)
- In reading operation in the pulsing types “Auto cycle” (adjustable pulse/pause ratio) or “free.”

If timeout is activated, it will have no effect here.

Important!

The CLV61x has no optical indicator (LED) for laser diode activity.

Maintenance and Care

The CLV61x operates without the need for maintenance, except for cleaning the reading window if it gets contaminated.

- In order to obtain maximum reading performance from the CLV61x, the reading window must be checked for contamination at regular intervals (e.g., weekly). This applies especially when using the CLV61x in harsh environments (dust, abrasion, moisture, etc.).
For reading, the reading window has to be generally dry.

Cleaning the Reading Window

The type of screen material used in the reading window can be found on the type label of the device:

CLV61x-xxxxy

- y = 0: Glass
- y = 1: Plastic

NOTE

Damage to the Reading Window!

Reduced reading performance due to scratches or streaks on the reading window.

- Do NOT use any aggressive cleaning agents with powder additives (increased abrasion) or agents e.g., acetone for cleaning.
- Avoid any movements that could cause scratches or abrasions on the reading window.

1. Switch off the device for the duration of the cleaning (laser protection!) or if this is not possible, wear laser protection goggles, which absorb the wavelength used and effectively prevent damage to the eyes.
2. Remove dust from the reading window (glass) using a soft clean brush.
Plastic reading windows must **only** be wet-cleaned!
3. Clean the reading window (plastic /additionally for glass if required) with a clean, soft, damp cloth (mild, anti-static cleaning agent).

Important!

If the reading window is scratched or damaged (cracked, broken), the window must be replaced by SICK service personnel. Contact SICK Service to arrange this.

Static charge causes dust particles to adhere to the reading window. This effect can be avoided by using the SICK anti-static plastic cleaner (no. 5600006) in combination with the SICK lens cloth (no. 4003353).

Transport and Storage

The CLV61x must be transported and stored in its original packaging. The device must not be stored in airtight containers, so that any residual moisture is able to escape.
Storage conditions: dry, dust-free. no direct sunlight, -20 ... +70 °C (-4 ... +158 °F), relative air humidity max. 90% (non-condensing).

Repairs

Repair work on the CLV61x may only be performed by qualified and authorized service personnel from SICK AG.

Disassembly and Disposal

At the end of the life time cycle, any CLV61x which can no longer be used must be disposed of in an environmentally friendly manner in accordance with the respective applicable country-specific waste disposal regulations. The CLV61x is electronic waste and must under no circumstances be disposed of with general waste! SICK AG is not currently able to take back devices that can no longer be used.

- Switch off the CLV61x before disassembly and physically disconnect it from the power supply.

Sources for Obtaining Additional Information

Additional information about the CLV61x and its optional accessories can be found in electronic form in the following places:

“Identification & Measuring Software & Manuals” DVD (no. 2039442)

CLV61x in General

- Technical information for CLV61x bar code scanners in German (no. 8015591) and English (no. 8015592)
- These operating instructions in German (no. 8015588) and English (no. 8015589), in other languages if applicable
- SOPAS ET configuration software with online help
- Ordering information in the product information for CLV61x bar code scanners in German (no. 8015420) and English (no. 8015421)
- Identification solutions product catalog
- Publications dealing with accessories

Integration of CLV61x in SICK CAN Sensor Network

- SICK CAN sensor network operating instructions in English

Integration of CLV61x FIELDBUS in PROFIBUS

- CDF600-21xx PROFIBUS fieldbus module operating instructions in German (no. 8015334) and English (no. 8015335)
- Technical information for CDF600-21xx PROFIBUS fieldbus module (no. 8015336) and English (no. 8015337)

Product Web Page for the CLV61x (www.mysick.com/en/clv61x)

- Suitable accessories
- Detailed technical specifications (online data sheet)
- Dimensional drawing and 3D CAD dimension models in various electronic formats
- Reading field diagrams
- Identification solutions product catalog
- CLV61x product information
- EC Declaration of Conformity
- SOPAS ET configuration software updates
- Online help for SOPAS ET as a PDF
- CLV61x bar code scanner operating instructions in German (no. 8015588) and English (no. 8015589), in other languages if applicable
- Technical information for CLV61x bar code scanners in German (no. 8015591) and English (no. 8015592)
- All publications contained on the aforementioned DVD (via links)

Documents on Request

- Overview of command strings

Support is also available from your sales partner: www.sick.com/worldwide